



Xenon light source



Microfluidic  
Reagent Rotor



Ready-to-Use reagents.  
No warm-up period  
required.

**7** minutes

Sample-to-answer in  
3 simple steps and  
approximately 7-10 minutes

**18** month


18-month  
shelf life

**27** tests

Up to 27 tests  
in a single run

## Clinical Chemistry<sup>+</sup>

Chemistry Analyzer Celercare<sup>®</sup> V5

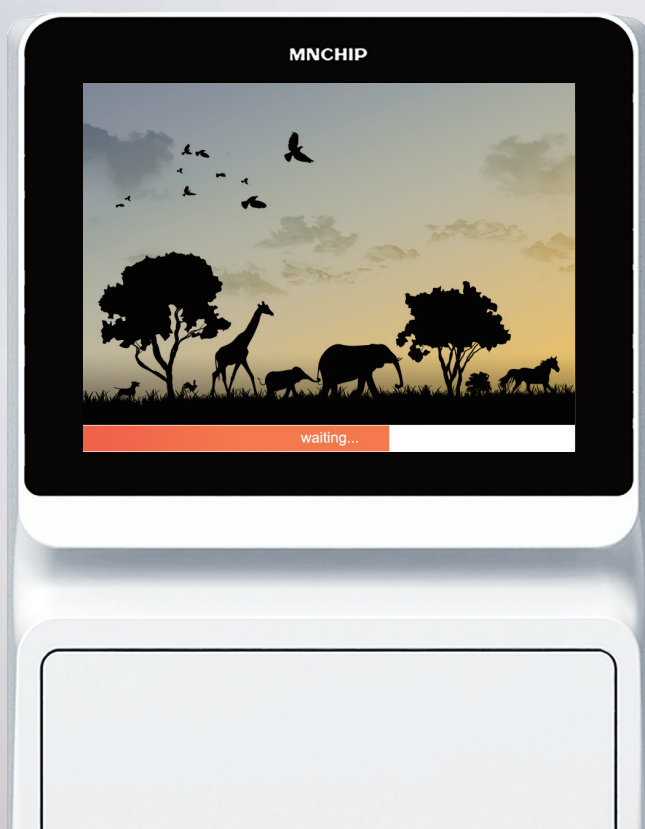

**MNCHIP**

